


upper arm with "artery" mark positioned directly over the brachial artery. The bottom edge of the cuff should be positioned approximately one inch above the ante-cubital fold. Wrap the end of the cuff, not containing the bladder, around arm snugly and smoothly and engage adhesive strips. To verify a correct fit, check that the INDEX line falls between the two RANGE lines.

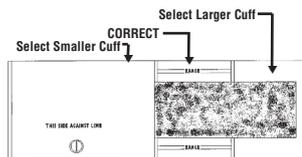

3. Inflate the cuff

Close the ADFLOW™ valve by turning thumbscrew clockwise.

Palpate the radial artery while inflating the cuff. Be sure to inflate cuff quickly by squeezing bulb rapidly. Inflate cuff 20-30mmHg above the point at which the radial pulse disappears.

4. Position the Stethoscope

Position the chestpiece in the antecubital space below the cuff, distal to the brachium. Do not place chestpiece underneath the cuff, as this impedes accurate measurement. Use the bell side of a combination stethoscope for clearest detection of the low pitched Korotkoff (pulse) sounds.

5. Deflate the cuff

Open the valve to deflate the cuff gradually at the AHA recommended rate of 2-3mmHg per second.

6. Measurement

Record the onset of Korotkoff sounds (Phase 1) as the systolic pressure, and the disappearance of these sounds (Phase 5) as the diastolic pressure. (Some healthcare professionals prefer recording diastolic 1 and diastolic 2. Diastolic one occurs at phase 4).

After measurement is completed, open valve fully to release any remaining air in the cuff. Remove cuff.

Care and Maintenance

Warning: Before transporting this instrument, mercury must be stored in the tank and the reservoir lock **MUST** be switched to the off position to prevent mercury spills.

Storage

After measurement, wrap cuff around bulb and store in base of main unit. **IT IS NOT NECESSARY TO CLOSE UNIT AFTER EACH USE - HOWEVER, ALWAYS REMEMBER TO LOCK MERCURY WITHIN THE RESERVOIR BEFORE CLOSING LID.**

Manometer Periodically replace the filter plug and diaphragm, and clean the inside of the plastic cartridge tube using alcohol and a lint free pipe brush. Units should be cleaned and serviced periodically depending on frequency of use, or whenever inside of cartridge tube appears dirty. Proper servicing of your mercury unit according to a strict maintenance schedule will assure maximum measurement accuracy and extend the life of your instrument.

For directions on disassembling the unit refer to the enclosed schematic diagram and accompanying instructions.

PLEASE NOTE: MERCURY IS TOXIC. SECURE MERCURY WITHIN THE RESERVOIR BEFORE SERVICING UNIT. ALWAYS WEAR PROTECTIVE CLOTHING (GLOVES AND GOGGLES) WHEN CLEANING OR SERVICING THE UNIT. CLEAN ANY SPILLED MERCURY PROMPTLY USING APPROVED MERCURY CONTAINMENT KITS. ONLY PROPERLY TRAINED SERVICE TECHNICIANS SHOULD ATTEMPT TO SERVICE THE UNIT. CONSULT THE ENCLOSED MANUAL ENTITLED "JUST IN CASE" FOR PROCEDURES ON DEALING WITH A MERCURY SPILL.

Limited Warranty

American Diagnostic Corporation (ADC) warrants its products against defects in materials and workmanship under normal use and service as follows:

1. Warranty service extends to the original retail purchaser only and commences with the date of delivery.

Symbols

Symbol	Definition	Symbol	Definition
	Important Warning/Caution		Manufacturer's Information
	Not made with natural rubber latex		Temperature Limit
	Circumference Size		Humidity Limitation

Device Description and Intended Use

ADC® aneroid sphygmomanometers are used by professional healthcare providers and individuals trained in auscultatory blood pressure technique to determine systolic and diastolic blood pressure in humans and animals.

A warning statement in this manual identifies a condition or practice which, if not corrected or discontinued immediately could lead to patient injury, illness, or death.

- **CAUTION:** Federal law restricts this device to sale by or on the order of a physician or licensed healthcare practitioner.
- **WARNING:** If luer lock connectors are used in the construction of tubing, there is a possibility that they might be inadvertently connected to intra-vascular fluid systems, allowing air to be pumped into a blood vessel. Immediately consult a physician if this occurs.
- **WARNING:** Do not allow a blood pressure cuff to remain on patient for more than 10 minutes when inflated above 10 mmHg. This may cause patient distress, disturb blood circulation, and contribute to the injury of peripheral nerves.
- **WARNING:** Safety and effectiveness with neonate cuff sizes 1 through 5 is not established.
- **WARNING:** Do not twist connectors when joining the blood pressure cuff to tubing as this may cause the connectors to stick and make changing the blood pressure cuff difficult.
- **WARNING:** When using with an infant or child cuff, extra care must be taken to prevent over-inflation. With smaller cuffs (infant or child) the cuff can inflate to over 300mmHg with just two full compressions of the bulb. To prevent discomfort or injury to the patient and damage to the

2. The entire sphygmomanometer is warranted for one year.
3. The inflation system is warranted for three years.
4. The calibrated plastic cartridge tube is warranted for life and will be replaced FREE OF CHARGE when returned freight prepaid with the complete unit.

What Is Covered: Calibration, repair or replacement of parts, and labor.

What is Not Covered: Transportation charges to and from ADC. Damages caused by abuse, misuse, accident, or negligence. Incidental, special, or consequential damages. Some states do not allow the exclusion or limitation of incidental, special, or consequential damages, so this limitation may not apply to you.

To Obtain Warranty Service: Send item(s) postage paid to ADC, Attn: Repair Dept., 55 Commerce Drive, Hauppauge, NY 11788. Please include your name and address, phone no., proof of purchase, with a brief note explaining the problem, and \$2.00 to cover the cost of return shipping and handling.

Implied Warranty: Any implied warranty shall be limited in duration to the terms of this warranty and in no case beyond the original selling price (except where prohibited by law). This warranty gives you specific legal rights and you may have other rights which vary from state to state.

To register your product visit us at
www.adctoday.com/register

FOR QUESTIONS, COMMENTS, OR SUGGESTIONS
CALL TOLL FREE:
1-800-ADC-2670 OR VISIT www.adctoday.com/feedback

This manual is available online in a variety of languages,
follow the links for language options.
www.adctoday.com/care




55 Commerce Drive
Hauppauge, N.Y. 11788, U.S.A.
www.adctoday.com

IB p/n 9353-00 - rev 9

Printed in the U.S.A.

DIAGNOSTIX™ 922 MERCURIAL BLOOD PRESSURE INSTRUMENT

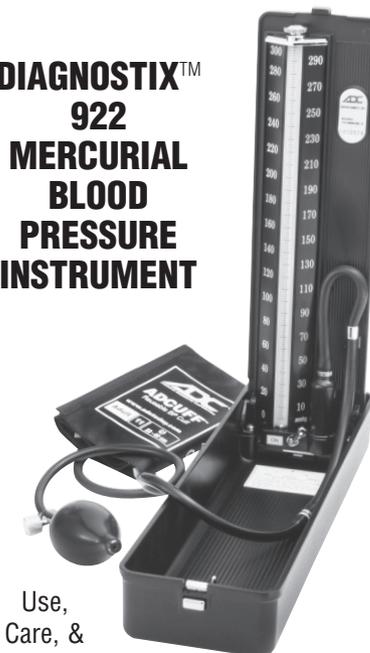

Use,
Care, &
Maintenance



A Special Thank You...

Thank you for choosing an ADC blood pressure instrument. We're proud of the care and quality that goes into the manufacture of each and every sphygmomanometer that bears our name.

Only the finest materials are used to assure you of a timeless instrument designed for optimum performance.

You'll quickly appreciate the results for you now own the finest sphygmomanometer that money can buy.

With proper care and maintenance your ADC blood pressure instrument is sure to provide you with many years of dependable service. Please read the following instructions and general information which will prove helpful in allowing you to enjoy your ADC product.

Thank you for your patronage. It is indeed our pleasure to serve you.

Sincerely,
American Diagnostic Corp.

instrument, bulb should be partially squeezed, so that each "stroke" inflates the cuff in 40mmHg to 60mmHg increments until inflated to the desired level.

- **WARNING:** This product may contain a chemical known to the state of California to cause cancer, birth defects, or other reproductive harm.

Parts and Assembly

This booklet contains operating and maintenance information for the DIAGNOSTIX™ 922 series desktop mercurial blood pressure instrument. Please read and retain.

Your DIAGNOSTIX™ 922 consists of a main unit with 4mm calibrated unbreakable plastic cartridge tube, inflation system (which includes the ADCUFF™ nylon cuff with Size Guide™ marking system, latex-free inflation bladder, bulb, and the ADFLOW™ valve), luer connector, and operating instructions.



Connecting the Inflation System to Manometer

Remove the red cap which seals the reservoir containing mercury. Attach the free end of reservoir tube securely to air inlet. Save red safety cap for later use. When transporting mercury instrument we recommend replacing the red safety cap.

Please note: It is normal for negligible amounts of residual mercury droplets to accumulate around the air inlet beneath the red safety cap during transportation.

Warning: Before transporting this instrument, mercury must be stored in the tank and the reservoir lock **MUST** be switched to the off position to prevent mercury spills.

Operating Instructions

Your DIAGNOSTIX™ 922 Desktop Mercury Sphygmomanometer incorporates a special safety feature that locks the mercury within the reservoir during storage, transport, or maintenance.

To Operate the 922: To release the mercury from the reservoir, move the locking lever to the left. Mercury will flow up into the plastic cartridge tube and rest at the "0" mark. If the mercury doesn't rise within the tube, tilt the entire unit 45° to the left. If mercury fails to rise, or doesn't reach the "0" level, have unit serviced.

To Lock Mercury within the Reservoir: Tilt the entire unit back 45° towards the reservoir to permit mercury to flow out of cartridge tube and into reservoir. When cartridge tube is completely emptied of ALL mercury (and while it is still tilted 45°), move locking lever to the right. Mercury should be locked within the reservoir during maintenance or transport.

PLEASE NOTE: MERCURY SHOULD BE SECURED WITHIN THE RESERVOIR BEFORE CLOSING LID, DURING TRANSPORT, OR WHEN SERVICING THE CARTRIDGE TUBE, DIAPHRAGMS, OR FILTERS. NEVER DISASSEMBLE UNIT UNLESS MERCURY IS FIRST LOCKED WITHIN RESERVOIR.

MEASUREMENT PROCEDURE

1. Patient Position

The patient should sit or lie comfortably. The arm should be fully supported on a flat surface at heart level. (If the arm's position varies, or is not level with the heart, measurement values obtained will not be consistent with the patient's true blood pressure.) Observer should view manometer in a direct line and at eye level to avoid "parallax error."

2. Apply the cuff

ADCUFF™ nylon cuffs, with proprietary Size Guide™ marking system, are specially designed to promote the precise, accurate determination of blood pressure. Index and range markings ensure use of the correct cuff size. The artery mark indicates proper cuff positioning. Place the cuff over the bare